

$SEP_{max} = 3.07 \text{ mmol/L}$


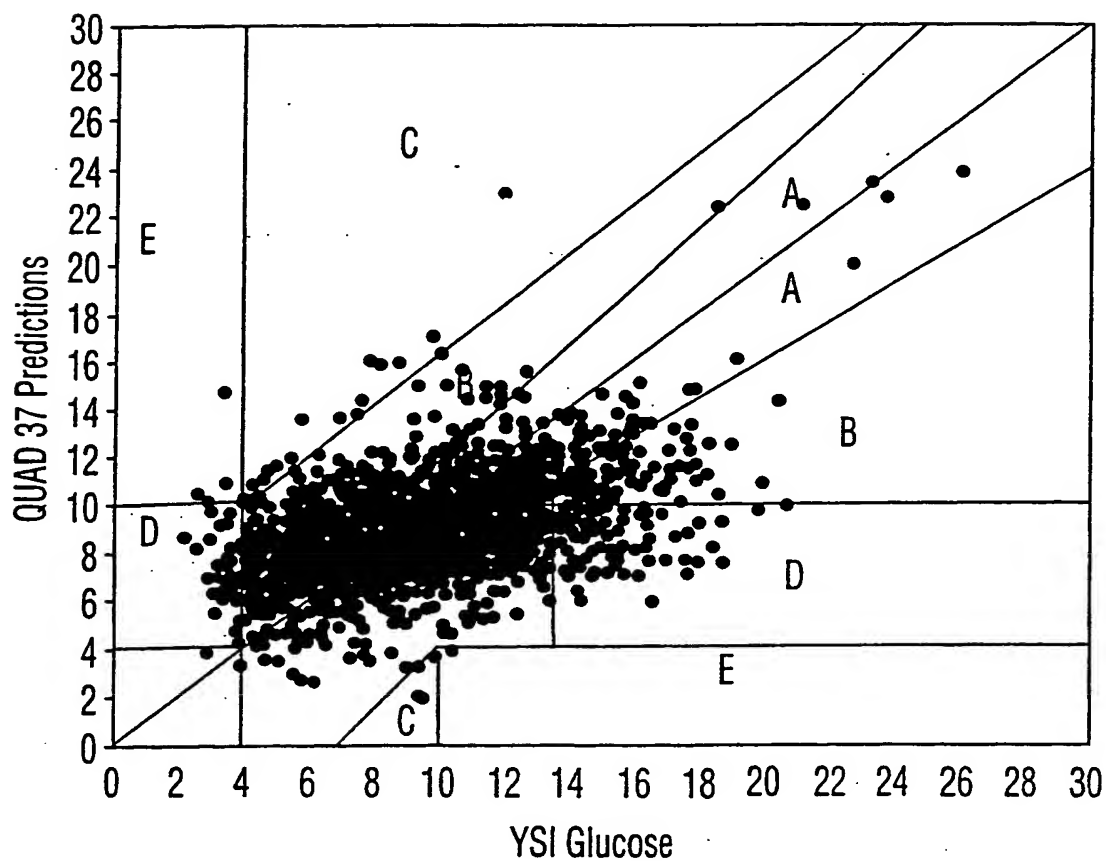


FIGURE 1

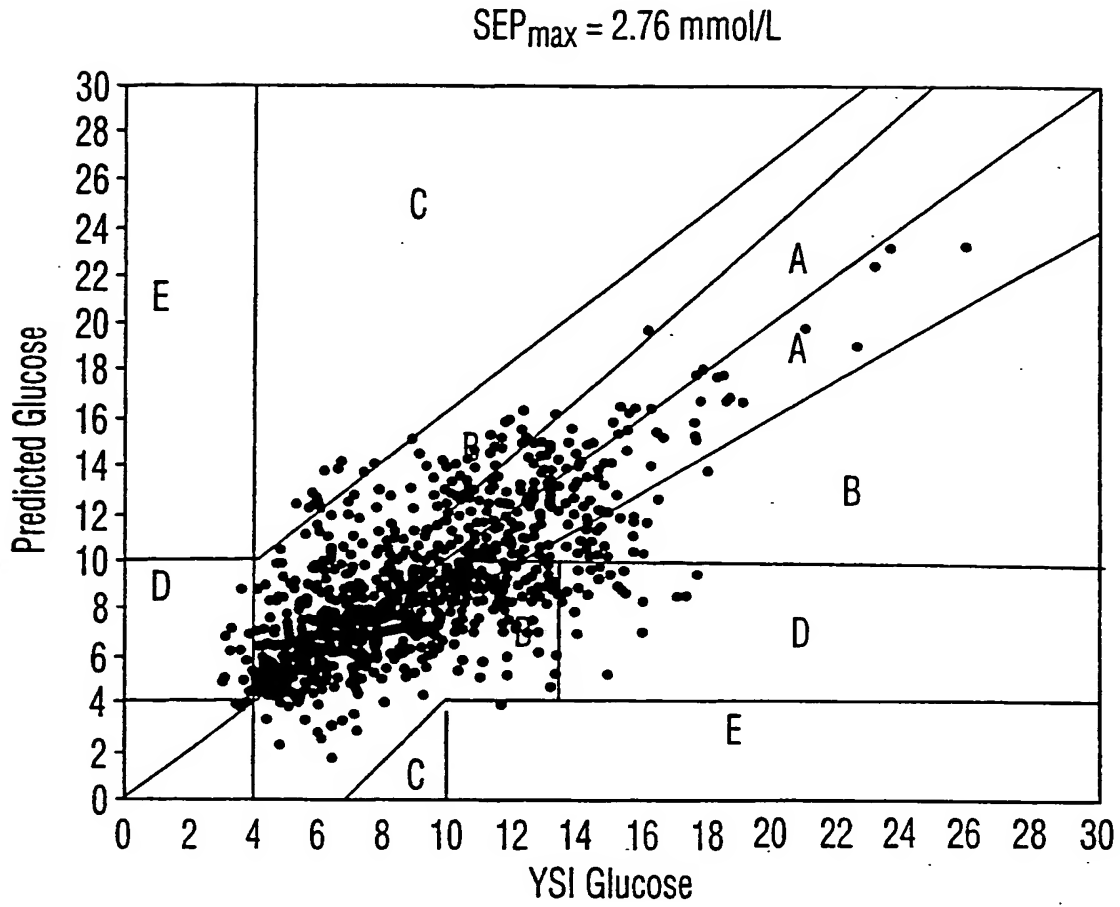


Clarke Error Grid

Zone	%
A	52.24
B	43.37
C	1.07
D	3.22
E	0.10

FIGURE 2

$SEP_{max} = 2.28 \text{ mmol/L}$

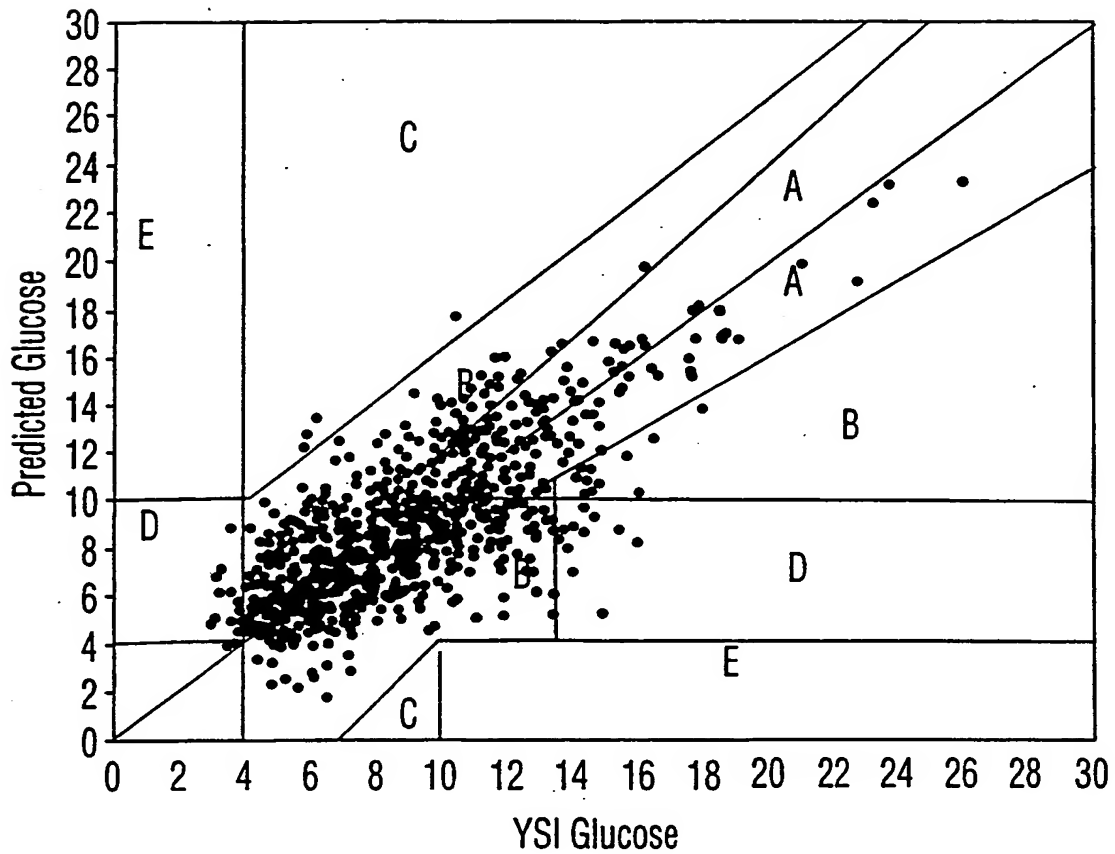

Clarke Error Grid

Zone	%
A	54.11
B	43.31
C	0.49
D	1.96
E	0.12

FIGURE 3

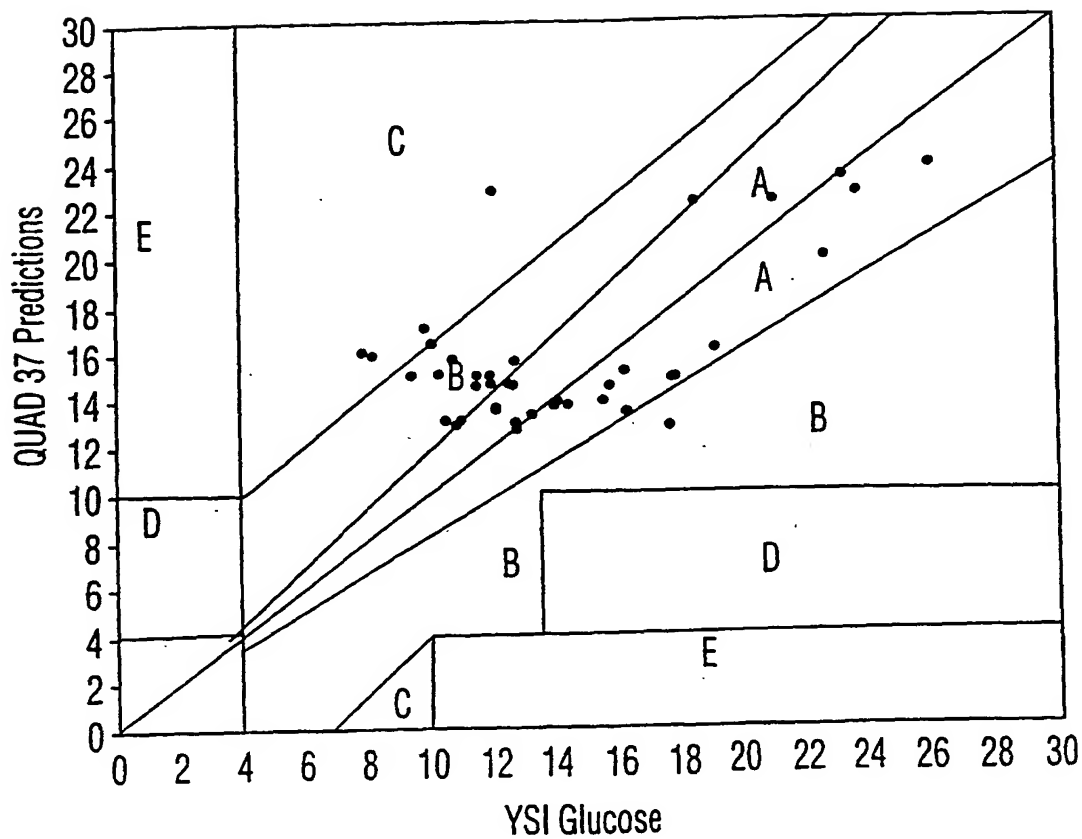


FIGURE 4

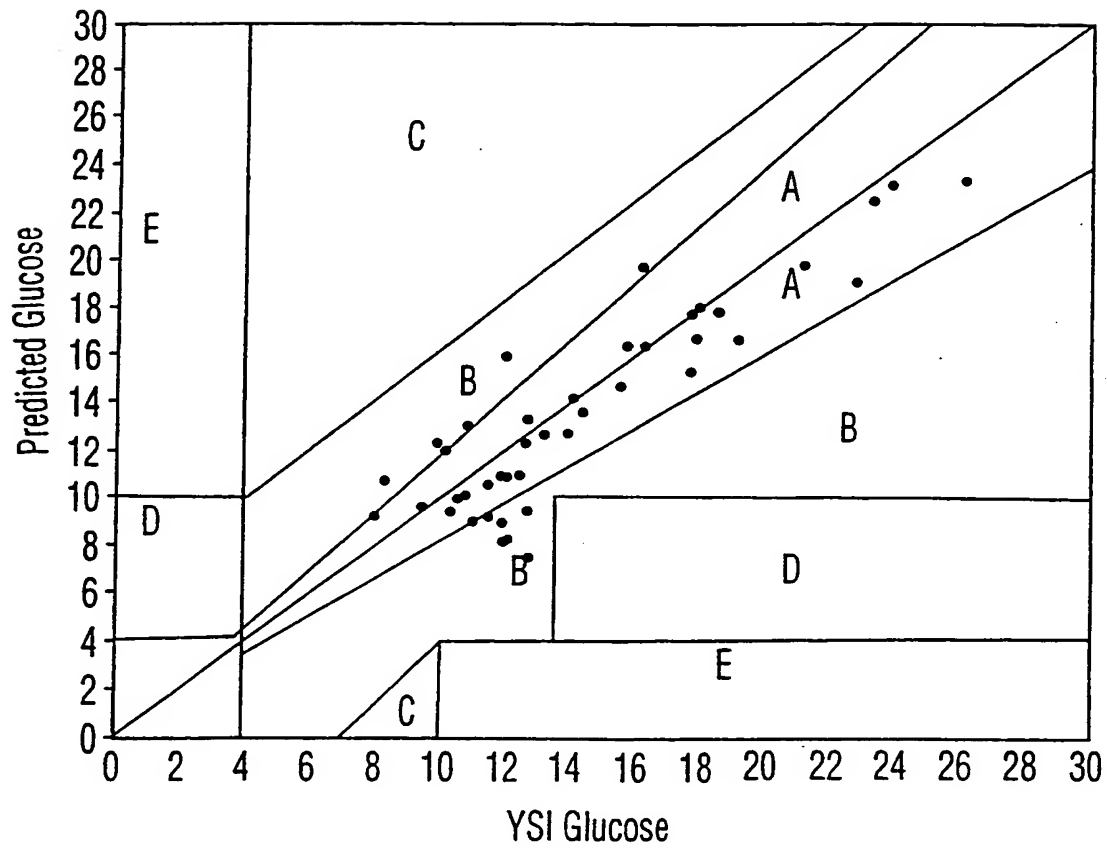


FIGURE 5